



LMA® Protector™ Airway with Cuff Pilot™ Technology

Revolutionizing Airway Access

The LMA® Protector™ Airway is the most advanced second generation airway from Teleflex.

Dual gastric channels

The only laryngeal mask that combines a pharyngeal chamber and dual gastric drainage channels, designed specifically to channel gastric content away from the airway.

Silicone

The airway tube and cuff are 100% silicone, phthalate free and designed to conform to the anatomy. Silicone cuffs have been shown to reduce risk of sore throat¹ and achieve higher seal pressures² compared with PVC cuffs.

Cuff Pilot™ Technology

An integrated cuff pressure indicator for single-use airway management devices that enables continuous cuff pressure monitoring at a glance and facilitates easy, accurate adjustment when necessary.^{3,4}

Second Seal Technology

The elongated cuff facilitates the upper esophageal seal.

Ability to intubate

Allows direct intubation using visual guidance.

Benefits



The Clinician

Excellent seal pressures, dual gastric channel and continuous cuff pressure monitoring inspires confidence.



Your Institution


Designed to help reduce airway-related complications and improve procedural efficiencies.



The Patient

Phthalate free silicone cuff designed for patient comfort.

LMA® Protector™ Airway with Cuff Pilot™ Technology

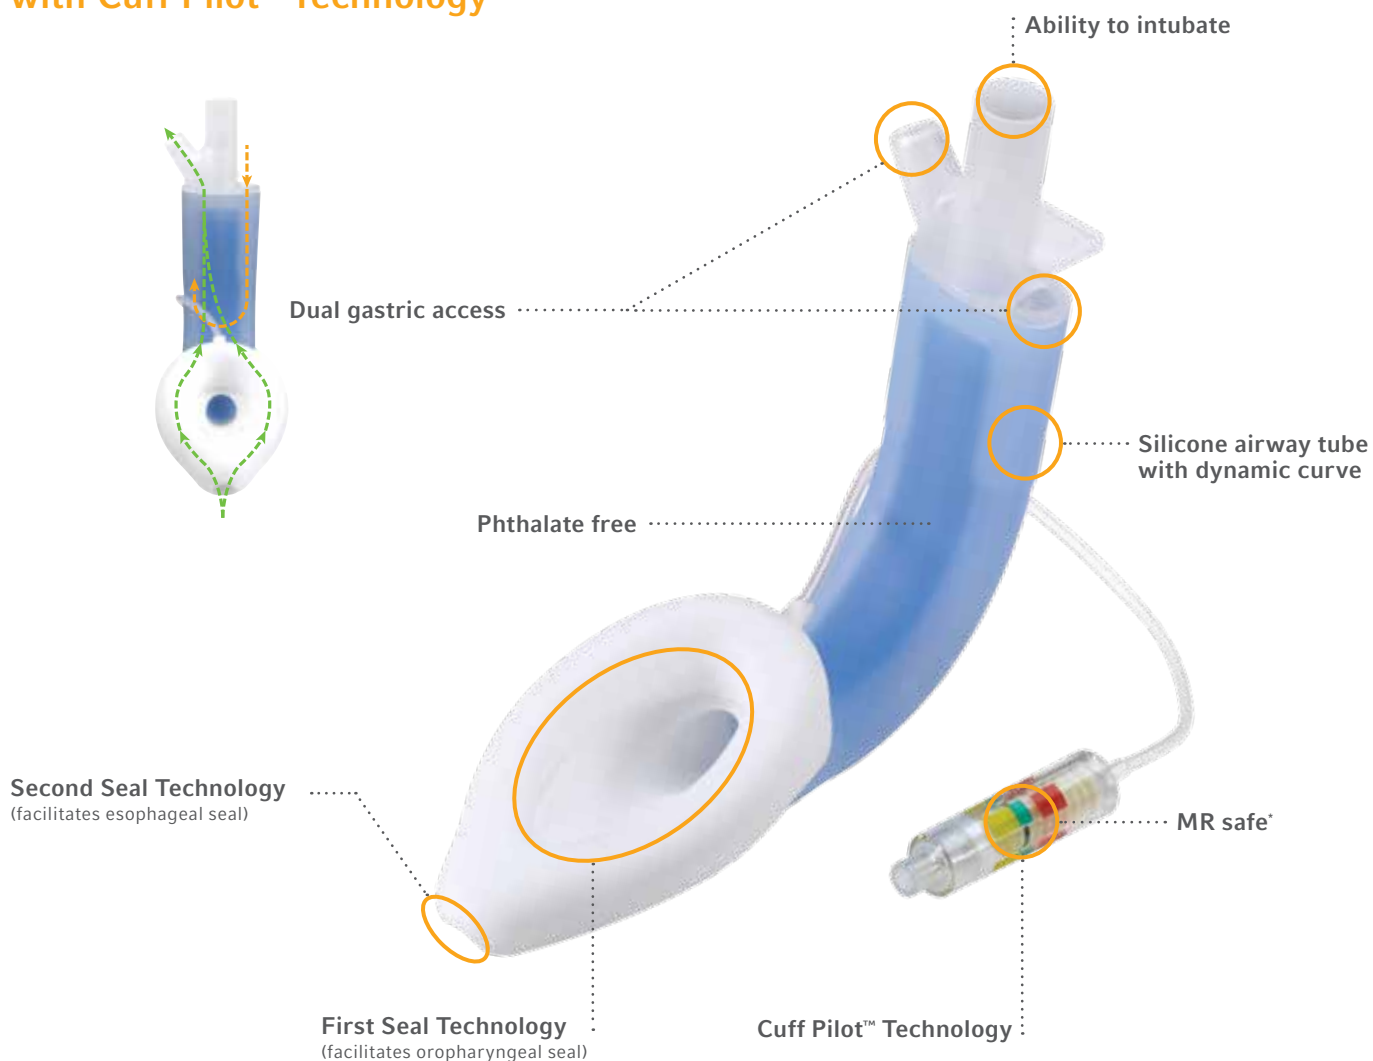

LMA® Protector™ Airway with Cuff Pilot™ Technology

| MASK SIZE | PRODUCT CODE WITH CUFF PILOT™ TECHNOLOGY | PRODUCT CODE WITH PILOT BALLOON | PATIENT WEIGHT IN KG | MAXIMUM INTRACUFF PRESSURE** IN CM H ₂ O | MAXIMUM ETT ID IN MM | LARGEST SIZE OG TUBE IN FR. |
|-----------|--|---------------------------------|----------------------|---|----------------------|-----------------------------|
| 3 | 192030 | 195030 | 30-50 | 60 | 6.5 | 16 |
| 4 | 192040 | 195040 | 50-70 | 60 | 7.5 | 18 |
| 5 | 192050 | 195050 | 70-100 | 60 | 7.5 | 18 |

ETT=ENDOTRACHEAL TUBE | OG=OROGASTRIC TUBE

* LMA® Protector™ Airway with Cuff Pilot™ Technology only.

** It is recommended that the cuff be inflated to a maximum intracuff pressure of 60 cm H₂O.

References:

1. William A, Chambers NA, Erb TO, Ungern-Sternberg BS. Incidence of sore throat in children following use of flexible laryngeal mask airways – impact of an introducer device. *Pediatric Anesthesia*. 2010;839-843. [Pubmed: 20716076].
2. Jagannathan N, Sohn LE, Sawardekar A, Gordone J, Langen KE, Anderson K. A randomized comparison of the LMA Supreme and LMA ProSeal in children. *Anaesthesia*. 2012;67:632-639. [Pubmed: 22420717].
3. Martin DP et al. Clinical evaluation of a novel LMA with a color-coded pressure gauge. *Int J Pediatr Otorhinolaryngol*. 2013;77(1):76-78.
4. Wong DT et al. New supraglottic airway with built-in pressure indicator decreases postoperative pharyngolaryngeal symptoms: a randomized controlled trial. *Can J Anaesth*. 2013;60(12):1197-1203.

Teleflex, Cuff Pilot, First Seal, LMA, LMA ProSeal, LMA Protector, LMA Supreme and Second Seal are trademarks or registered trademarks of Teleflex Incorporated or its affiliates, in the U.S. and/or other countries. Information in this document is not a substitute for the product Instructions for Use. The products in this document may not be available in all countries. Please contact your local representative. All data current at time of printing (04/2016). Subject to technical changes without further notice.

© 2016 Teleflex Incorporated. All rights reserved. PBE-2500-004 REV B IW 201605



www.lmaco.com

Teleflex

Distributed by:

Teleflex Headquarters International, Ireland · Teleflex Medical Europe Ltd. · IDA Business & Technology Park
Dublin Road · Athlone · Co Westmeath · Tel. +353 (0)9 06 46 08 00 · Fax +353 (0)14 37 07 73 · orders.intl@teleflex.com
www.teleflex.com